



OLP-39G/-39X

**SmartPocket™ V2
TruePON Tester**

User manual

BN 2336/98.11

2022.11

English

Please direct all inquiries to your local Viavi sales company.
The addresses can be found at:

www.viavisolutions.com/en-us/contact-sales-expert

The description of additional features of the device can be found at:
www.viavisolutions.com/en-us/products/network-test-and-certification

Copyrights

This product or parts of this product are based on recommendations and/or standards from the standardization section of the International Telecommunication Union – ITU-T and/or the European Telecommunications Standards Institute – ETSI. These recommendations and standards are subject to the proprietary rights of these organizations. It is not permitted to copy ITU-T recommendations or ETSI standards fully or in part and/or to pass them on to third parties without prior written permission from ITU-T and/or ETSI.

Copyright

© Copyright 2022 Viavi Solutions Inc. All rights reserved.
Viavi and the Viavi logo are trademarks of Viavi Solutions Inc.
All other trademarks and registered trademarks are the property of their respective owners.

Viavi Solutions Deutschland GmbH
Arbachtalstraße 5, 72800 Eningen u. A., Germany

Order number: BN 2336/98.11

Issue: 2022.11

Previous issue: 2022.04

Notes:

Changes may be made to specifications, designations and delivery information.

CONTENTS

INTRODUCTION	5
OLP-39G/-39X TruePON Tester	5
User manual update	6
Symbols used in this user manual	7
SAFETY INFORMATION	9
GETTING STARTED	10
Unpacking the device	10
Device overview	11
Power Supply	12
Switching the device on/off	15
Selecting a power mode	15
Selecting a measurement mode	15
DISPLAY OVERVIEW	16
Status bar	16
PON mode	16
TruePON mode	17
ONT Detection mode (Option)	18
PON MODE	19
Selecting an operation mode	19
Selecting a display mode	20
Absolute power level mode	20
Loss mode	21
Pass/Fail mode	22
TRUEPON MODE	23
Selecting an operation mode	23
Selecting a Pass/Fail display mode	24
Setting the ODN class	25
Performing a TruePON measurement	26
Recalling measurement results	26
ONT DETECTION MODE (OPTION)	27
Selecting an operation mode	27
Detecting the ONT serial number	28

SETTINGS	29
The Settings menu	29
Changing settings	30
MEMORY MANAGEMENT	31
General information	31
Storing measurements	31
Recalling measurements	31
Deleting measurements	32
DATA EXPORT AND FIRMWARE UPDATE	33
USB and SmartReporter	33
Bluetooth® and MobileTech app /	
StrataSync cloud (future application)	33
MAINTENANCE	34
Cleaning the test port	34
Cleaning the instrument	35
SPECIFICATIONS	36
OLP-39G/-39X	36
General specifications	36
ORDERING INFORMATION	38
OLP-39G, OLP-39X	38
Calibration report	38
Accessories	38
Smart Reporter	38
PRODUCT REGULATORY COMPLIANCE	39

1 INTRODUCTION

OLP-39G/-39X TruePON Tester

The OLP-39G/-39X is a specialized TruePON Tester designed for use cases such as system/network qualification, subscriber activation, and troubleshooting of passive optical network (PON). The instrument performs wavelength selective optical power measurements suitable for testing G-PON networks, as defined in ITU-T G.983/4 or IEEE 802.3ah (OLP-39G) and XGS-PON networks, as defined in ITU-T G.9807.1 respectively (OLP-39X). In TruePON mode the OLP-39G/-39X identifies the OLT-ID, ODN class, and loss based on the TOL (Transmitted Optical Level from OLT), while the ODN class can be recognized automatically or set manually.

An integrated pass/fail analysis feature simplifies standard conformity and optical budget/margin testing, and provides unambiguous measurement result presentation.

With PC-based reporting, all test results can be summarized in a professional, industry-proven report.

Main features

The OLP-39G/-39X offers many helpful features that are optimized to workflows of typical telecom operators, and thus ensure that test times are kept as short as possible.

- OLT-ID, ODN class and loss based on TOL for G-PON (OLP-39G) and XGS-PON (OLP-39X)
- Display of G-PON and XGS-PON results separately or simultaneously (OLP-39X)
- Accurate and repeatable wavelength selective power measurements
- Unambiguous pass/fail result presentation and user definable pass/fail thresholds
- Data storage for up to 1000 measurements
- USB-C interface for measurement data transfer to a laptop/PC
- Easy operation and instantly ready to operate
- Versatile power supply options using dry or rechargeable batteries or via the USB-C interface
- Automatic power-off (can be disabled)
- Color-coded test head cover for easy distinction between APC and PC connector types
- Smart-Reporter PC software for data management and report generation

Description of OLP-39G and OLP-39X features in this manual

In this user manual the OLP-39X with G-PON and XGS-PON is described. Please note that for the OLP-39G only G-PON is available.

User manual update

If the operating instructions about features provided by your device are missing, please visit the Viavi web site to check if additional information is available.

To download the latest operating instructions:

1. Visit the Viavi web site at www.viavisolutions.com.
2. Search for **SmartPocket**.
3. Open the download area and download the operating instructions if available.

Symbols used in this user manual

Various elements are used in this user manual to draw attention to special meanings or important points in the text.

Symbols and terms used in warnings

The following warnings, symbols and terms are used in this document in compliance with the American National Standard ANSI Z535.6-2011:

NOTICE

Follow the instructions carefully to avoid **damage to or destruction of the instrument**.

⚠ CAUTION

Follow the instructions carefully to avoid a low or medium risk of **injury to persons**.

⚠ WARNING

Follow the instructions carefully to avoid **potential death or severe injury** to persons.

⚠ DANGER

Follow the instructions carefully to avoid **death or severe injury** to persons.



High Voltage

Follow the instructions carefully to avoid **damage** to the instrument or **severe injury** to persons.

This safety instruction is given if the danger is due to **high voltage**.



Laser

Follow the instructions carefully to avoid **damage** to the instrument or **severe injury** to persons.

This safety instruction is given if the danger is due to **laser radiation**. Information specifying the laser class is also given.

Warning format

All warnings have the following format:

WARNING

Type and source of danger

Consequences of ignoring the warning

- Action needed to avoid danger.

The following character formats are used in this user manual:

✓	Requirement This requirement must be met first; e.g. ✓ The device is switched on.
► 1. 2.	Instruction Follow the instructions given (the numbers indicate the order in which the instructions should be followed); e.g. ► Select mode.
<i>Italics</i>	Result Indicates the result of following an instruction; e.g. <i>The page opens.</i>
Bold type face	Pages, controls, and display elements Screen pages, controls, and display elements are indicated in bold type.
Text in blue	Cross references Cross references are indicated in blue type. When using the PDF version, just click on the blue text to skip to the cross reference.
[MODE]	Device keys Device keys are indicated within square brackets.
	The three sensitive keys are indicated as squares, the active key is highlighted.

2 SAFETY INFORMATION



- ▶ All safety information for your device can be found in the printed booklet “Safety, Disposal and Environmental Protection” provided with your device.
- ▶ Carefully read and follow all instructions given there.



- ▶ The booklet “Safety, Disposal and Environmental Protection” is attached to this PDF. You can open it from the attachment window or by clicking the thumbnail on the left.

3 GETTING STARTED

Unpacking the device

Packing material

We suggest that you keep the original packing material. It is designed for reuse (unless it is damaged during shipping). Using the original packing material ensures that the device is properly protected during shipping.

Checking the package contents

Your device is shipped with the following accessories:

- 2.5 mm universal adapter
- 2 dry batteries AA
- User manual
- Belt bag

Checking for shipping damage

After you unpack the device, check to see if it has been damaged during shipping. This is particularly likely if the packaging is visibly damaged. If there is damage, do not attempt to operate the device. Doing so can cause further damage. In case of damage, please contact your local Viavi Sales Company. Addresses can be found at www.viavisolutions.com.

Recovery following storage/shipping

Condensation can occur if a device that is stored or shipped at a low temperature is brought into a warm environment. To prevent damage, wait until no more condensation is visible on the surface of the device before powering it up. Do not operate the instrument until it has reached its specified temperature range and wait until it has cooled down if the instrument was stored at a high temperature (see [“Environmental conditions” on page 37](#)).

Device overview



1 Test head cover

2 Fixed SC adapter

3 Display

4 Key pad

Representation in the user manual:

[■ □ □] Context sensitive keys (here left key is selected)

[MODE] Mode/Settings key

[📁] Save/Results key

[⏻] Power key

5 USB interface

For power supply and measurement data downloads and updates.

6 Battery compartment (on rear of the device)


Keys

The key pad contains two types of keys:

- **Context sensitive keys:** The functions of these keys depend on the selected mode or menu and is shown in the display above the key.
- **Function keys:** The functions of these keys are always the same and shown on the key itself.

Key usage (first and second function levels)

The function keys and the context sensitive keys in certain modes have two function levels.



A second function level is indicated by two cascading frames.

- **Short press:** Select the first level function.
- **Long press:** Holding the key for at least 2 sec. opens the second level. You then have access to additional functions or a menu to change settings.

	Short press	Long press
	Press to switch the device on/off.	
Context keys 	Functions depend on selected mode and display. See following chapters for more information.	
MODE key 	Toggle between PON mode and TruePON mode	Open the settings menu.
Save/Result key 	Store the current measurement.	Open the list of saved measurements.

Power Supply

NOTE: The devices are not designed for batteries based on lithium.

The following power sources can be used to operate the OLP-39G/-39X:

- Two 1.5 V dry batteries (Mignon AA size, alkaline type recommended)
- Two 1.2 V NiMH rechargeable batteries (Mignon AA size)
- via AC adapter over USB interface

Battery operation

⚠ WARNING

Dangers in handling batteries

Handling batteries may be dangerous. Please note the following safety instructions.

- ▶ Please note the battery operation safety information in the booklet “**Safety, Disposal and Environmental Protection**” provided with your device.

Replacing the batteries

- ▶ Do not replace individual batteries. Always change both batteries at the same time.
- ▶ Always use batteries of the same type; i.e. do not mix rechargeable and non-rechargeable batteries.

Replacing the batteries

The battery compartment is on the back of the device.

1. Pull down the lid to open the battery compartment.

NOTICE:

Take care to insert the batteries correctly.

The correct polarity is indicated by a diagram inside the battery compartment.

2. Insert new batteries or replace dead ones.
3. Close the battery compartment.
4. Press [⏻] to switch on.

NOTE: The batteries cannot be recharged with the OLP-39G/-39X.

General tips on using batteries

- Never use batteries based on lithium.
- Always handle batteries with care.
- Do not drop or damage the batteries or expose them to excessively high temperatures.
- Do not store rechargeable batteries for more than one or two days at very high temperatures (e.g. in a vehicle), either separately or fitted in the device.
- Do not leave discharged batteries in the device for a long time if it is not being used.
- Do not store rechargeable batteries for more than 6 months without recharging them at intervals.
- Avoid deep discharging of the batteries as this can cause the cell polarity to reverse and make the battery useless.

Protecting the environment

Please dispose of any unwanted dry batteries and rechargeable batteries carefully. They should also be removed from the instrument if it is to be scrapped. If facilities in your country exist for collecting waste or for recycling, please make use of them rather than throwing the batteries in the normal trash. You will often be able to return used batteries to the place where you purchase new ones. Any dry or rechargeable batteries that you purchased from Viavi can be returned to one of our Service Centers for disposal.

Operation from AC power

To fit one of the mains plug adapters:

- ▶ See [Fig. 1](#) and follow the instructions which are shown on the packaging of the mains plug adapter.

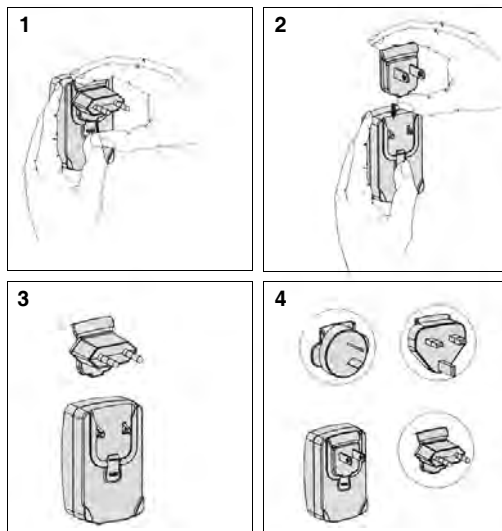


Fig. 1 Fitting the mains plug adapter

To operate the OLP-39G/-39X from AC power:

1. Connect the USB-C connector power cord to the OLP-39G/-39X.
2. Plug the mains plug adapter into the AC receptacle.

Switching the device on/off

The OLP-39G/-39X has two battery power modes:

Mode	Icon	Description
Permanent ON (PERM)		The device is switched on permanently.
Automatic OFF (ECON)		The device switches off 20 minutes after the last operation. This function is only available when the device is powered from batteries.

To switch the device on/off:

- Press **[⊙]** to switch the device on/off.

Selecting a power mode

- ✓ The device is switched on.
- 1. Long press **[MODE]** to open the settings menu.
- 2. Use **[↑↓]** to select **ECON**.
- 3. Press **[]** to select power mode:
ON = ECON
OFF = PERM
- 4. Press **[MODE]** to close the menu.

Selecting a measurement mode

- ✓ The device is switched on.
- Short press **[MODE]** to toggle between **PON**, **TruePON** and **ONT Detection** mode.

4 DISPLAY OVERVIEW

Status bar

PON	Selected mode: PON, TruePON, ONT Detection	
	Bluetooth® is active Bluetooth connection allows for data transfer via the MobileTech app (for future use).	
7:15	Real Time Clock Time can be changed via the settings menu.	
	Battery status in PERM power mode: Device remains switched on.	
	Battery status in ECON power mode: Device switches off 20 min. after last operation.	
	The device is powered via USB	

PON mode

NOTE: XGS-PON and Dual mode are available in OLP-39X only.

G-PON	Shows wavelength and power level of G-PON and XGS-PON	
XGS-PON	Shows measurement results in dBm, dB or W.	
dBm	Shows measurement results in dBm, dB or W.	
Dual	Shows selected mode Press key to select mode: 1490 nm > 1577 nm > Dual > ...	
Abs>Ref	Press key to set current measurement value as new reference level.	
dBm	Short press key to select mode: dBm/Watt > Loss > PF Abs > PF Loss > ... Long press key to toggle unit: dBm <> Watt	


Fig. 2 XGS-PON (top),
Dual mode (bottom)

TruePON mode

NOTE: In this examples **DUAL** mode is selected.
XGS-PON and Dual mode are available in OLP-39X only.


Home screen

Showing PON values before starting the OLT-ID detection

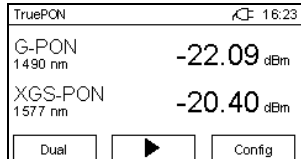G-PON / XGS-PON	Shows wavelength and power level of G-PON and XGS-PON	 The screenshot shows the TruePON interface with a battery icon and time 16:23. It displays G-PON 1490 nm at -22.09 dBm and XGS-PON 1577 nm at -20.40 dBm. At the bottom are buttons for Dual, a right arrow, and Config.
Dual	Press key to select operation mode: Dual > G-PON > XGS-PON > Dual >...	
	Short press key to start measurement Long press key to recall last results	
Config	Press key to change TruePON settings	

TruePON overview

Showing detected OLT-IDs after pressing the start button.

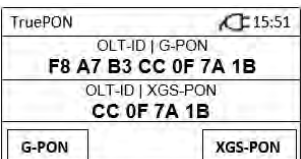OLT-ID G-PON	Shows OLT-ID of G-PON in ASCII code	 The screenshot shows the TruePON interface with a battery icon and time 15:51. It displays OLT-ID G-PON as F8 A7 B3 CC 0F 7A 1B and OLT-ID XGS-PON as CC 0F 7A 1B. At the bottom are buttons for G-PON and XGS-PON.
OLT-ID XGS-PON	Shows OLT-ID of XGS-PON in HEX code	
G-PON	Press key to show G-PON details	
XGS-PON	Press key to show XGS-PON details	

TruePON details

Showing details of detected OLT-IDs.

Header	Selected PON type	 The figure shows two screenshots of the TruePON details screen. The top screenshot is for G-PON, showing OLT-ID HEX as F8 A7 B3 CC 0F 7A 1B, Loss as 23.20dB, ODN-Class as C+, and Power as -22.36dBm. The bottom screenshot is for XGS-PON, showing OLT-ID HEX as CC 0F 7A 1B, Loss as PASS, ODN-Class as PASS, and Power as PASS. Both screens have buttons for AUTO/ONT and N1.
OLT-ID	OLT-ID in ASCII or HEX code	
Loss	Loss in dB or Pass/Fail	
ODN-Class	ODN class as detected or Pass/Fail	
Power	Power in dBm or Pass/Fail	
Footer	AUTO/N1: ODN-Class (Auto or as set) ONT: Location as set	
NOTE: In the Settings menu Pass/Fail can be individually enabled or disabled for Loss, ODN-Class, and Power.		Fig. 3 P/F Off (top), P/F ON (bottom)

ONT Detection mode (Option)

NOTE: XGS-PON and Dual mode are available in OLP-39X only.

Home screen

Showing PON values before starting the ONT detection

G-PON / XGS-PON	Shows wavelength and power level of G-PON and XGS-PON	
Dual	Press key to select operation mode: Dual > G-PON > XGS-PON > Dual > ...	
	Short press key to start measurement Long press key to recall last results	

ONT Detection Summary

Showing detected ONT Serial Number and ID.

OLT-ID G-PON	Shows OLT-ID of G-PON in ASCII code	
OLT-ID XGS-PON	Shows OLT-ID of XGS-PON in HEX code	
ONT Serial Number	Shows the serial number of the detected ONT	
ONT ID	Shows the ID of the detected ONT	
Status	Shows the status of the detected ONT: ACT = Activated: The ONT is activated and working DEAC = Deactivated: Client ist still waiting for approval	

5 PON MODE

- ▶ Short press **[MODE]** to toggle between **PON**, **TruePON** and **ONT Detection** mode.

NOTE: XGS-PON and Dual mode are available in OLP-39X only.

Selecting an operation mode

The OLP-39G/-39X provides three operation modes with following displays:

- **G-PON:** Gigabit Passive Optical Network measurement at 1490 nm
- **XGS-PON:** 10-Gigabit-Capable Symmetric Passive Optical Network measurement at 1577 nm
- **Dual:** Display of G-PON and XGS-PON simultaneously

To select an operation mode:

- ▶ Press **[■□□]** to select a mode.

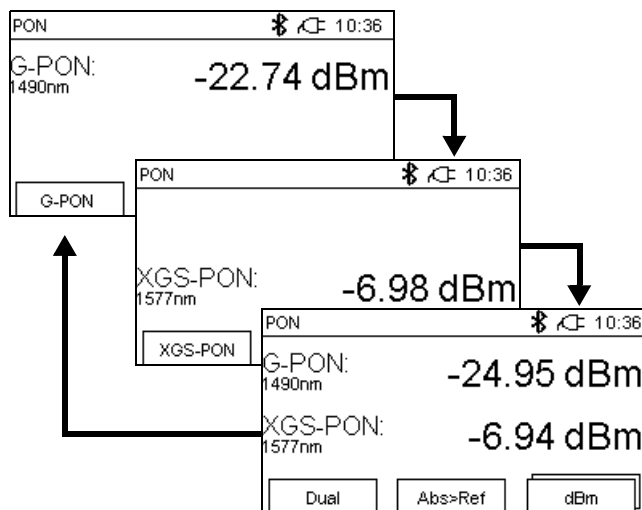


Fig. 4 Operation modes


Selecting a display mode

The OLP-39G/-39X provides following display modes:

- **dBm/Watt:** Display of absolute power level
- **Loss:** Display of power level relative to a reference value
- **PF Abs:** Pass/Fail indication based on an absolute power threshold
- **PF Loss:** Pass/Fail indication based on a relative power threshold

To select a display mode:


- ▶ Press [☐☐☐☒>] to toggle between the displays modes.

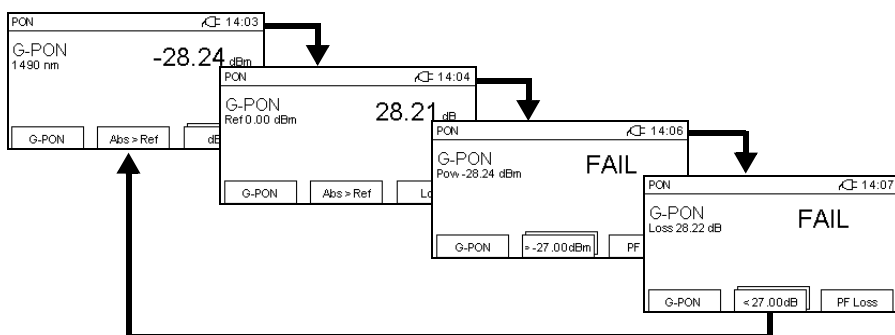

Absolute power level mode

The power level is displayed in dBm or Watts (nW, μ W, mW).

- ▶ Long press [☐☐☐☒>] to toggle dBm/Watts.

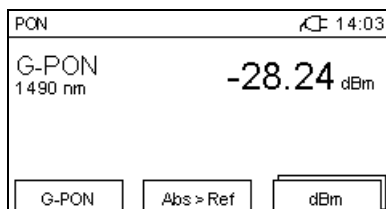

NOTE: The context sensitive field shows the selected unit.

Loss mode

In **Loss** mode the power level relative to a reference value is displayed. The reference value can be set by defining the current power level as the reference value [**Abs>Ref**].


- Press [☐☐☒] to display relative power level.

Setting the reference level

- ✓ **Absolute power level** mode or **Loss** mode is selected.

- Press [**Abs>Ref**].

The current power level is set as the new reference level.

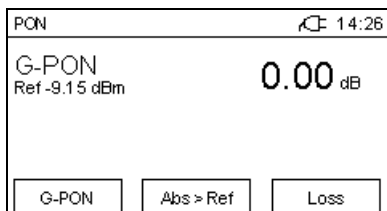

NOTE: The reference level can be stored for both wavelength separately.
When **Dual** is selected, the power levels of both wavelengths are set as reference level simultaneously.

Pass/Fail mode

An integrated pass/fail analysis feature simplifies standard conformity testing and provides unambiguous measurement result presentation.

The OLP-39G/-39X provides two Pass/Fail modes:

- **PF Abs:** Pass/Fail indication based on a absolute power threshold
- **PF Loss:** Pass/Fail indication based on a loss threshold

To select a Pass/Fail mode:

- ▶ Press [☐☐☐☐] until **PF Abs** or **PF Loss** is displayed.

NOTE: When **PF Abs** or **PF Loss** is selected the two modes can also be toggled by pressing [☐☐☐☐].


Setting the PASS threshold

Setting the fail threshold is identical for both Pass/Fail modes.

- ✓ **PF Abs** or **PF Loss** mode is selected. Press [☐☐☐☐] to toggle between both modes.

1. Press [☐☐☐☐] to select a wavelength (see also page 19).
2. Long press [☐☐☐☐].

The Set Fail Threshold screen opens.

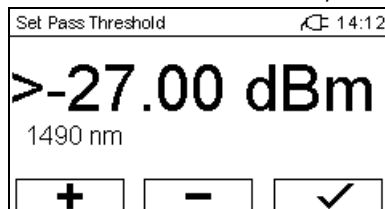

3. Use [+]/[-] to change the threshold.
4. Press [✓] to save the new threshold.

NOTE: When Dual mode is active, the fail threshold can not be set. Select G-PON or XGS-PON to set threshold individually.

6 TRUEPON MODE

- ▶ Short press **[MODE]** to toggle between **PON**, **TruePON** and **ONT Detection** mode.

NOTE: XGS-PON and Dual mode are available in OLP-39X only.

Selecting an operation mode

The OLP-39G/-39X provides three operation modes with following displays:

- **G-PON:** Gigabit Passive Optical Network measurement at 1490 nm
- **XGS-PON:** 10-Gigabit-Capable Symmetric Passive Optical Network measurement at 1577 nm
- **Dual:** Display of G-PON and XGS-PON simultaneously

To select an operation mode:

- ▶ Press **[■□□]** to select a mode.

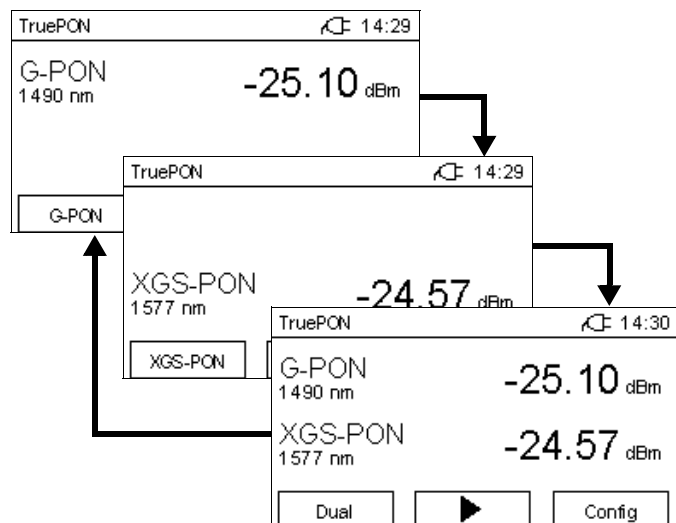


Fig. 5 Operation modes

Selecting a Pass/Fail display mode

The OLP-39G/-39X provides two display modes:

- **P/F On:** Display of Pass/Fail results
- **P/F Off:** Display of absolute measurement results

TruePON G-PON 15:51			TruePON XGS-PON 15:51		
OLT-ID HEX F8 A7 B3 CC 0F 7A 1B			OLT-ID HEX CC 0F 7A 1B		
Loss 23.20dB	ODN-Class C+	Power -22.36dBm	Loss PASS	ODN-Class PASS	Power PASS
AUTO		ONT	N1		ONT

Fig. 6 Display modes: P/F **Off** (left), P/F **On** (right)

To select a display mode:

1. In the **Home** screen press [□□■].
The Config dialog opens, P/F is selected.

TruePON Configuration 15:56	
Pass / Fail	OFF
Location	ONT
ODN Class G-PON	Auto
ODN Class XGS-PON	N1
↑	↓
Toggle	

2. Press [□□■] to select **ON** or **OFF**.
3. Short press **[MODE]** key to close dialog.

Individual Pass-Fail-settings

Even if P/F is set to **On**, the Pass/Fail display for Loss, ODN-Class and Power can be disabled.

For example:

You want Pass/Fail results for Loss and Power, but want to disable Pass/Fail indication for the ODN class.

TruePON G-PON 15:51		
OLT-ID HEX F8 A7 B3 CC 0F 7A 1B		
Loss 23.20dB	ODN-Class C+	Power -22.36dBm
AUTO		ONT

- See [“Memory Management” on page 31](#) how to change the individual Pass/Fail settings.

Setting the ODN class

The ODN class can be set to **Auto** or an specific class individually for G-PON and XGS-PON.

To set the ODN class:

1. In the **Home** screen press the **Config** key.
*The **Config** menu opens.*

TruePON Configuration  15:56	
Pass / Fail	OFF
Location	ONT
ODN Class G-PON	Auto
ODN Class XGS-PON	N1
↑ ↓ Toggle	


2. Press  or  to select **G-PON** or **XGS-PON**.
3. Press  to step trough the ODN classes:
 - **G-PON**: Auto > B > B+ > C > C+ > D > Auto >...
 - **XGS-PON**: Auto > N1 > N2 > E1 > E2 > Auto >...
4. Press **[MODE]** to close the menu.

Performing a TruePON measurement

To get TruePON measurement results a TruePON measurement must be started.

To perform a measurement:

- ✓ Set ODN class (see “Setting the ODN class” on page 25).
- ✓ Select Pass/Fail display mode (see “Selecting a Pass/Fail display mode” on page 24).
- 1. In the **Home** screen short press [☐☒☐] to start measurement. *The running measurement is displayed on the screen.*

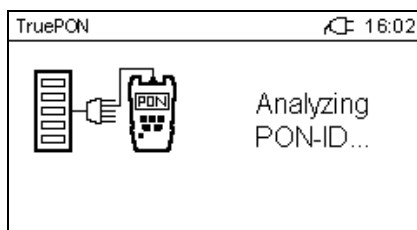

*If **Dual** was selected, the ONT-IDs are displayed in an overview. If G-PON or XGS-PON was selected, the measurement details are displayed immediately.*

TruePON 15:51		TruePON G-PON 15:51		
OLT-ID G-PON F8 A7 B3 CC 0F 7A 1B		OLT-ID HEX F8 A7 B3 CC 0F 7A 1B		
OLT-ID XGS-PON CC 0F 7A 1B		Loss 23.20dB	ODN-Class C+	Power -22.36dBm
☒ G-PON	☐ XGS-PON	AUTO ONT		

Fig. 7 Results display: overview (left), detail (right)

- 2. If **Dual** was selected, press [☒☐☐] or [☐☐☒] to display **G-PON** or **XGS-PON** measurement details.
- 3. Press [**MODE**] to return to the previous screen.

Recalling measurement results

After leaving the measurement details screen, the permanent measured power levels are displayed in the Home screen. From there the last TruePON measurement results can be recalled.

To recall the last measurement results:

- ✓ The Home screen is displayed.
- ▶ Long press [☐☒☐]. *The display is the same as after the starting the measurement.*

7 ONT DETECTION MODE (OPTION)

- ▶ Short press **[MODE]** to toggle between **PON**, **TruePON** and **ONT Detection** mode.

NOTE: XGS-PON and Dual mode are available in OLP-39X only.

Selecting an operation mode

The OLP-39G/-39X provides three operation modes with following displays:

- **G-PON:** Gigabit Passive Optical Network measurement at 1490 nm
- **XGS-PON:** 10-Gigabit-Capable Symmetric Passive Optical Network measurement at 1577 nm
- **Dual:** Display of G-PON and XGS-PON simultaneously

To select an operation mode:

- ▶ Press **[■□□]** to select a mode.

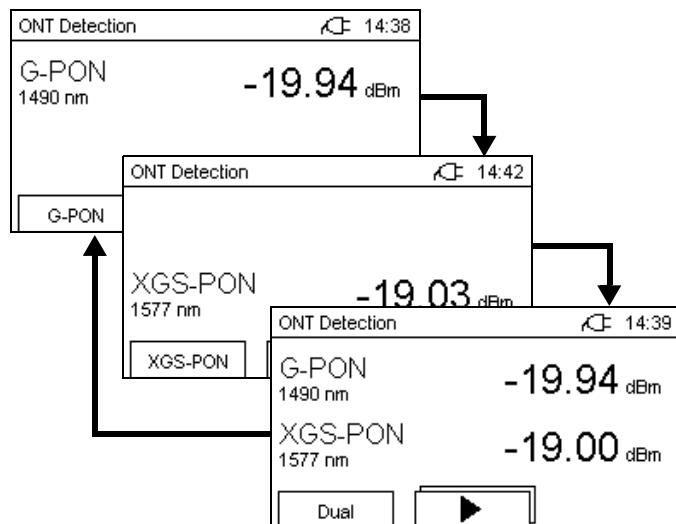



Fig. 8 Operation modes

Detecting the ONT serial number

The ONT serial number is detected bei unplugging and plugging the desired ONT. The OLP-39G/-39X listens to the information send from the OLT and displays the serial number and ID.


To detect the ONT serial number:

- ✓ The OLP-39G/-39X is connected to a free splitter port.
- ✓ Operation mode and is selected as desired.
- 1. In the **Home** screen short press [  ] to start measurement.
- 2. Unplug the connection to the desired ONT.

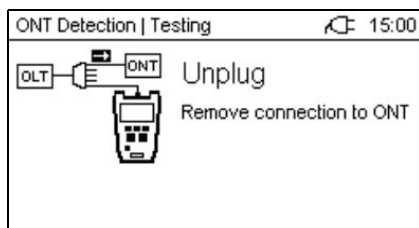

The unplug screen disappears after a few seconds.

- 3. Plug in the connection to the ONT again.

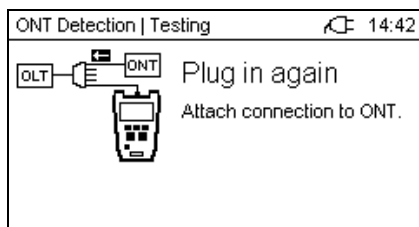

The summary is shown (depending on the selected PON type).

ONT Detection Summary			14:43
OLT ID		PON Type	
70 70 08 F2		XGS-PON	
ONT Serial Number		ONT ID	Status
AVMG6D3D2E89		1	ACT

- ▶ Press the **[MODE]** key to return to the **Home** screen.
- ▶ In the **Home** screen long press [  ] to recall the last detection results.

8 SETTINGS

In the Settings menu you can do the following:

- Change general instrument settings and reset all settings
- Change some basic TruePON settings
- Switch Bluetooth and economy mode on/off

The Settings menu

Item	Settings	Description
Hour	1 ... 12	Current time: Hour
Minute	1 ... 59	Current time: Minute
Year	2020 ... 2030	Current time: Year
Month	01 ... 12	Current time: Month
Day	01 ... 31	Current time: Day
About	–	Shows device data including last calibration date
Options	–	Shows the installed options.
Factory Reset	Reset	▶ Press [✓] to confirm setting. ▶ Press [↶] to return to the settings menu.
G-PON OLT-ID	ASCII/HEX	Display OLT-ID in ASCII oder HEX code ▶ Press [□□■] to toggle HEX/ACII
XGS-PON OLT-ID	ASCII/HEX	Display OLT-ID in ASCII oder HEX code ▶ Press [□□■] to toggle HEX/ACII
G-PON Custom Thr.	0 dBm ... -32 dBm	Set custom threshold for G-PON
XGS-PON Custom Thr.	0 dBm ... -25 dBm	Set custom threshold for XGS-PON
Bluetooth LE	ON/OFF	Switch Bluetooth LE on/off
Marginal Threshold	0 dB ... 2 dB	Select a dB value to define a window for the PASS/FAIL mode threshold. Measurement values for Loss or Absolute within this window will be displayed as "Marginal". Thus, in PASS/FAIL mode 3 results are available: PASS/Marginal/FAIL.
ECON	ON/OFF	ON = ECON, OFF = PERM

Changing settings

1. Long press the **[MODE]** key.
The Settings menu opens.

Settings	Bluetooth, Airplane, 10:36
Hour	00
Minute	00
Year	2021
↑	↓ +

2. Press **[■□□]** or **[□■□]** to select an entry.

To change a value:

- ▶ Press **[□□■]** to edit it.
 - Press once to change one step at a time.
 - Hold down the key to increase the step change rate.

To toggle between two settings:

- ▶ Press **[□□■]** to toggle settings.

To leave the Settings menu:

- ▶ Press **[MODE]** key to close the Settings menu.

9 MEMORY MANAGEMENT

General information


The OLP-39G/-39X allows you to save the measured power level values in a data memory and recall them as required.

Up to 1000 results can be stored.

NOTE: See also [“Specifications” on page 36](#) for additional data management tools.

Storing measurements


- Press **[H]** to save the current result.
The result is saved when “Saving...” appears on the display and below the name of the currently saved data.
The results are always stored with the current date-/timestamp (e.g. 2021-01-13T16-05-52, corresponding to January 13th 2021 at 16h:05min:52s)

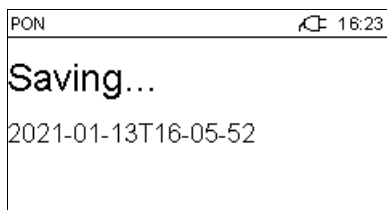


The new results are always appended successively at the last memory location, even if you clear a previously assigned memory location with a lower number.

Recalling measurements

1. Long press **[H]**.
The device shows the list of saved measurements.

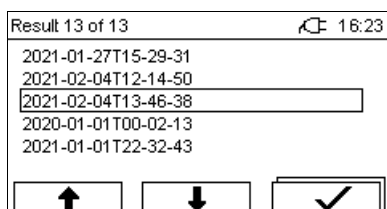

2. Press [**▲**]/[**▼**] to browse through the list.
3. Press [**✓**] to open the highlighted entry.
The selected measurement data is displayed.

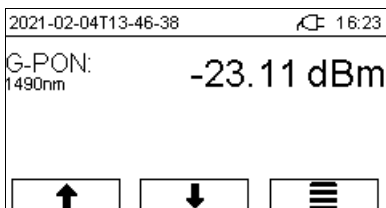


4. Press [**☰**] to return to the list or, press [**▲**]/[**▼**] to show next/previous result or press [**MODE**] to exit.


Deleting measurements

- ✓ The device shows the list of saved measurements.

1. If you want to delete a single entry, use [**▲**]/[**▼**] to select it.
2. Long press [**✓**] to open the sub menu.

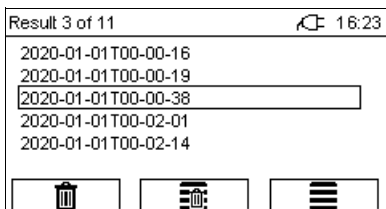

3. Press [**🗑**] to delete the selected entry, or press [**☰**] to delete all results.
A dialog will ask you to confirm the deletion.

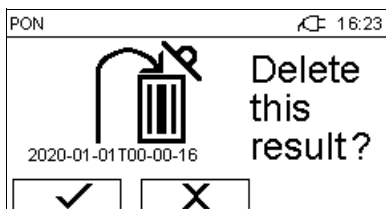

4. Press [**✓**] to accept or press [**X**] to cancel.
5. Press [**☰**] to close the sub menu and to show the list of saved measurements or press [**MODE**] to exit.

NOTE: You cannot select and overwrite empty memory locations.

10 DATA EXPORT AND FIRMWARE UPDATE

The USB interface or the Bluetooth® interface can be used for data export and firmware update.

USB and SmartReporter

When using the USB interface the SmartReporter allows you to easily transfer stored measurement data to a PC and to update the firmware.

The SmartReporter reporting tool always contains the latest Firmware Revision for all your SmartPocket™ devices. You can download the latest SmartReporter version for free from:

<https://updatemyunit.net/> > Application Software.

- ▶ For more information about data export and firmware update via USB and SmartReporter please refer to the SmartReporter user manual.
- ▶ If the USB interface is used in an environment with high electromagnetic radiation, please use a Ferrit shielded USB cable

Bluetooth® and MobileTech app / StrataSync cloud (future application)

You have also the choice to upload the saved data and to update the firmware using Bluetooth® via Viavi's MobileTech App into the StrataSync cloud.

- ▶ Please contact your Viavi representative for more information.

11 MAINTENANCE



⚠ WARNING

Invisible laser radiation

Maintenance or cleaning of the instrument while it is connected or operating may damage the instrument or injure you.

- ▶ Make sure that the instrument is switched off and disconnected from all power sources and optical radiation sources before maintenance or cleaning.
- ▶ Do not open the instrument for maintenance or service. Service shall be performed by Viavi trained personnel only.

Cleaning the test port

It is a good idea to check that the optical connections are clean and to clean them if necessary before starting measurements. Even very small dust particles on the end surfaces of the plugs or in the test adapters can adversely affect the accuracy of the measurement.

NOTICE

Damage to the photo diode

Touching the photo diode could scratch the glass surface.

- ▶ Be careful when cleaning the photo diode and do not use any rough cleaning materials.

1. Switch off the device.
2. Blow into the test adapter with compressed and clean air to remove dust.

NOTE: Cover the optical connections with the dust cap whenever they are not in use. This prevents them from getting dirty.

Cleaning the instrument

If the device gets dirty through use, you can clean it using a soft cloth moistened with a mild solution of detergent.

NOTICE

Water and cleaning fluids

The instrument may be damaged or destroyed if water or cleaning fluids penetrate it.

- Make sure that water or cleaning fluids do not get inside the instrument.
-

12 SPECIFICATIONS

OLP-39G/-39X

G-PON (1490 nm downstream)

Measurement range for power level	-35 to +10 dBm
Measurement Range for PON-ID	-30 to 0 dBm
Maximum power level	+20 dBm continuously +26 dBm <30 min.
Spectral range	1480 to 1500 nm
Measurement uncertainty	±0.5 dBm ¹⁾

1) At -10 dBm, at 23 °C ± 3 °C, at nominal wavelength

XGS-PON (1577 nm downstream, OLP-39X only)

Measurement range for power level	-35 to +10 dBm
Measurement Range for PON-ID	-25 to 0 dBm
Maximum power level	+20 dBm continuously +26 dBm <30 min.
Spectral range	1575 to 1580 nm
Measurement uncertainty	±0.5 dBm ¹⁾

1) At -10 dBm, at 23 °C ± 3 °C, at nominal wavelength

General specifications

Number of calibrated wavelengths	2 (1490 nm, 1577 nm)
Optical adapter system	Fixed SC

Memory

Data storage	1000 results
Data download capability	USB-C for PC transfer

Calibration interval

Recommended calibration interval	3 years
----------------------------------	---------

Power supply

Dry batteries	2x Mignon (AA) Alkaline 1.5 V (never use batteries based on lithium)
Power consumption	2.5 W max.
Operating life with dry/ rechargeable batterier	typ. 15 h (Bluetooth® off)
AC line operation	With separate 5 V DC USB adapter. Use EMC and Safety certified low energy adapters only.
Power saving	Auto power-off after approx. 20 min (can be disabled)

EMC and safety

Electromagnetic compatibility (EMC)	EN 61326-1:2020
Device safety	EN 61010-1:2010/A1:2019

Environmental conditions

Operating temperature range	-10 to +55 °C (14 to 131 °F)
Storage and transport	-40 to +70 °C (-40 to 158 °F)
Altitude	2000 m max. (6500 ft. max.)
Pollution degree	2
Ingress protection	IP44
Relative humidity up to +31 °C	15 to 85 %
Absolute humidity > +31 °C	1 to 29 g/m ³

Occasional condensation is tolerable as a limit condition.

Dimensions and weight

Dimensions (H x W x D)	30 x 80 x 150 mm (1.18 x 3.15 x 5.90 in)
Weight (incl. batteries)	200 g (0.44 lb)

13 ORDERING INFORMATION

OLP-39G, OLP-39X

OLP-39G - TruePON Tester Terminate Mode GPON	OLP-39G
OLP-39X - TruePON Tester Terminate Mode GPON and XGS-PON	OLP-39X

Calibration report

Calibration Report TruePON Testers (OLP-39G and OLP-39X)	2302/90.04
---	------------

Accessories

OCK-10 Cleaning Kit complete	2229/90.21
Alkaline batteries Mignon AA-Size LR6 (2 batteries required)	2229/90.01
USB 2.0 cable (Type A to Type C)	2212/2619
Universal AC Power Adapter	2302/90.01

Smart Reporter

Free download from www.updatemyunit.net/

14 PRODUCT REGULATORY COMPLIANCE



- **All information about the product regulatory compliance can be found in the printed booklet “Safety, Disposal and Environmental Protection” provided with your device.**



North America
Latin America
China
Germany

+1 844-468 4284
+1 954 688 5660
+86 21 6859 5260
+49 7121 86 0

Viavi product specifications and descriptions in this document are subject to change without notice.
© 2022